

## Keys to Successful Testing

Quality of sample analyzed = Quality of result

### Avoid vein collapse when drawing samples



- Minimize suction on the syringe, and do not draw back too quickly.

### Prevent hemolysis



- Use the largest vein and needle appropriate for blood collection.
- Never use any needle smaller than a 23 gauge size.



- Use minimal alcohol on fur/skin.



- Remove the needle from the syringe before dispensing into the blood tube, unless using a closed vacuum blood collection system.

### Ensure the correct ratio of anticoagulant to blood



- Always use the smallest collection tube needed.

- Fill lithium heparin and EDTA tubes to minimum fill line.



- Fill sodium citrate tubes exactly to the fill line.

### Prevent unwanted blood clotting



- Do not** hold off the vein for more than a few seconds before venipuncture.




- For feline samples collected from the medial saphenous vein: a vacuum blood collection system instead of a syringe is recommended.

### Do not allow samples to degrade



- Run the sample as soon as possible after drawing.


## Collection Tubes & Fill Order

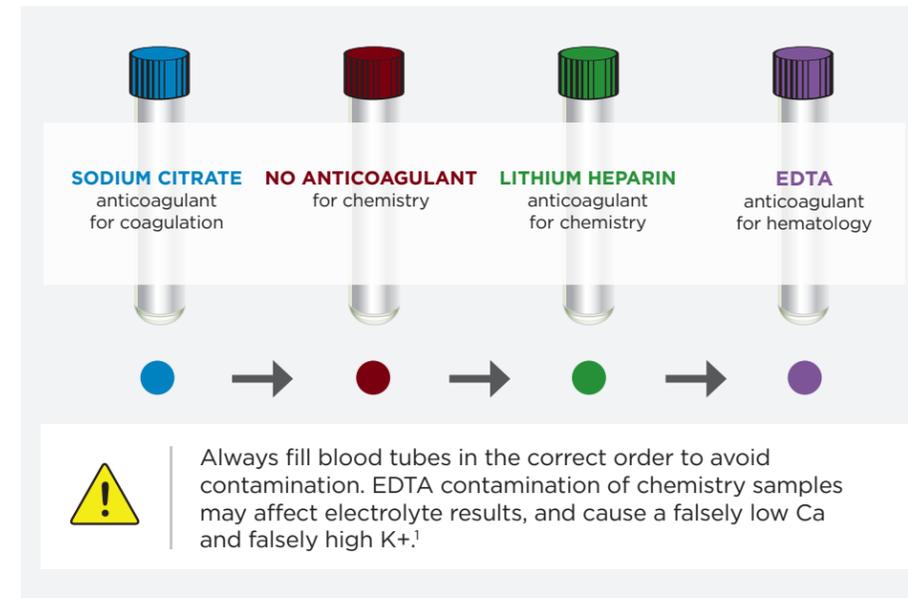

## Tube Handling


### Chemistry<sup>2,4</sup>

Whole blood samples must be inverted 8-10 times after collection and re-inverted just prior to use.

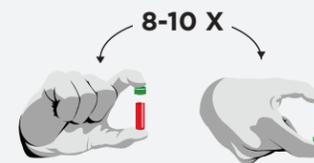

### Hematology<sup>3,4</sup>

Samples must be inverted 10-15 times after collection and re-inverted just prior to use.

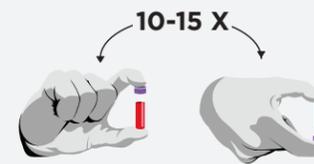

Never shake blood sample tubes.

1.3 mL and smaller tubes may need additional inversions for proper mixing.

Do not rely on a rocker to mix blood samples properly; rockers do not take the place of proper tube inversion.

## Sample Quality



**NORMAL** plasma and serum samples are straw colored, and do not have a yellow, red, or pink tinge.



**HEMOLYZED** plasma and serum samples have a pink/red tint due to broken red blood cells.

*Avoid hemolysis by using proper sample collection and handling techniques.<sup>1</sup>*



**LIPEMIC** plasma and serum samples have a milky appearance due to a high concentration of fat in the blood.

*Avoid lipemia by using a fasted patient sample whenever possible.<sup>1</sup> Remind clients to refrain from feeding their pets prior to their appointment.*



**ICTERIC** plasma and serum samples have a yellow color due to a disease or condition that causes excess bilirubin in the blood.



**CLOTTED** samples may have visible red clots that stick to wooden applicator sticks when swirled in a sample. Traumatic or delayed blood collection can lead to micro and /or macro clots.<sup>1</sup>

*Avoid clotted samples by inverting blood tube appropriately immediately after filling. Re-draw any clotted hematology samples.*

**NOTE:** Never run a clotted sample for analysis on the HM5.

## Sample Storage<sup>5,6</sup>



### Chemistry<sup>2</sup>

Lithium Heparin whole blood samples at room temperature\* must be run within 1 hour,<sup>8</sup> or separated to serum\* or plasma\* and run as soon as possible.<sup>7</sup> Serum and plasma samples may be stored refrigerated\*\* for up to 48 hours.<sup>8</sup>



### Hematology<sup>3</sup>

EDTA whole blood samples must be run within 1 hour at room temperature\*, and may be stored refrigerated\*\* for up to 12 hours.<sup>7</sup> Blood should return to room temperature prior to running on the HM5.

\* Stored plasma and serum samples must be separated and kept in a stoppered test tube containing no additive.

\*Room Temperature (68-77 °F)

\*\*Refrigerated Temperature (36-46 °F)

<sup>1</sup>Monti P, Archer J. Quality Assurance and Interpretation of Laboratory Data [Chapter 2]. BSAVA Manual of Canine and Feline Clinical Pathology. 3rd ed.; 2016: p. 12.

<sup>2</sup>VETSCAN VS2 Operator's Manual. 2013. 1200-7063 Rev. A. Data on file, ABX-00101

<sup>3</sup>VETSCAN HM5 Operator's Manual. 2018. 790-7013 Rev. F. Data on file, ABX-00248.

<sup>4</sup>Weiser, G. Laboratory Technology for Veterinary Medicine [Chapter 1]. Veterinary Hematology and Clinical Chemistry. 2012: p. 3.

<sup>5</sup>Wu, DW, et al., How Long can we Store Blood Samples: A Systematic Review and Meta-Analysis. EBioMedicine. 2017: p. 283-284.

<sup>6</sup>Kitchens, JL. Title The effects of the blood storage time on the accuracy of the comprehensive metabolic panel results. Maryville College, 2006.

<sup>7</sup>Monti P, Archer J. Quality Assurance and Interpretation of Laboratory Data [Chapter 2]. BSAVA Manual of Canine and Feline Clinical Pathology. 3rd ed.; 2016: p. 13.

<sup>8</sup>Weiser, G. Sample Collection, Processing, and Analysis of Laboratory Service Options [Chapter 2]. Veterinary Hematology and Clinical Chemistry, 2012: p. 36.